
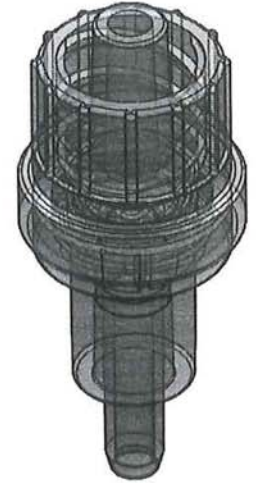



COUPE A-A

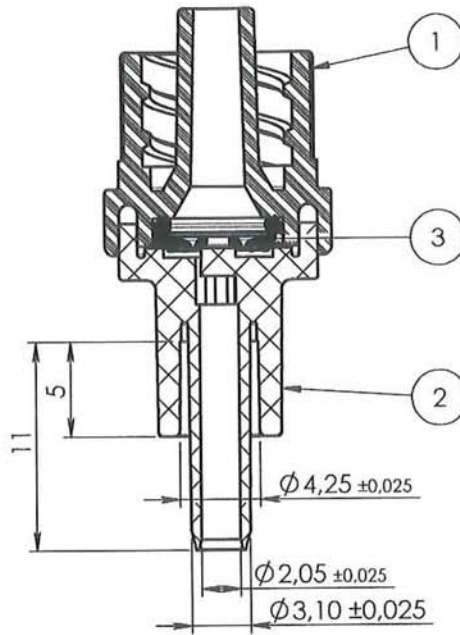

NOTA:

Rep	Matière	Code matière
1	SAN	M0376
2	ABS	M0480
3	Silicone	M0256

Checkvalve in stand by position:	Closed
Maximum retrograde leakrate:	≤ 0.1ml/h at a flow rate of 0.5ml/h
Position of use:	Independent
Priming:	Airbubbles completely removable
Approximate Priming volume:	0.15ml
Crack pressure:	≤ 12 mBar
Crack pressure after back pressure of 6 bar for 15 min:	≤ 20 mBar
Maximum back pressure:	6 Bar
Burst pressure (at room temperature in flow direction for 15 seconds air overpressure):	6 Bar
Flowrate with infusion set according to DIN 58362 with Glucose 40%:	≥ 90 ml/ min
Sterilization :	ETO-Gas, γ-irradiation up to 50 kGy
Material and dimensions :	See drawing

APPROBATION / APPROVAL		
Client / Customer :	Promepla Resp. BE :	Promepla Qualifié :
	<i>M. 08 15</i>	
Nom / Name, date & signature		

ORIGINAL


2	03/04/2014	BOUJMADA	Matière M0071 devient M0480, et code matière M0114 devient M0256, ajout du approximate priming volume	FOR021 : 5957
1	09/02/2011	RANDAZZO	Mise à jour cotation	
0	25/02/2008	BOUCHARD	Creation	
Rev.	Date	Designer	Modifications	N° Fiche FOR073 ou FOR021

Normes : ISO 594

Matière : VOIR NOTA

P. 1 / 1

Echelle : 5:2



Code matière : VOIR NOTA

Revision : 2

Format : A4

Reference : PBP22050

Tolérances générales :

Unités : mm, °, grs

Designation :
VALVE ABS TRANSP. - PRESSION OUVERTURE
12mBars - Ø 3x4.1mm - LLM

PROMEPLA

FOR035-1